

磁振影像學MRI 組織壓抑技術

盧家鋒 教授


國立陽明交通大學
生物醫學影像暨放射科學系
alvin4016@nycu.edu.tw



本週課程內容 <http://cflu.lab.nycu.edu.tw>

- 磁振造影流程
- 組織壓抑技術

- MRI The Basics (3rd edition)
 - Chapter 25: Tissue suppression techniques
- MRI in Practice, (4th edition)
 - Chapter 5: Pulse sequences
 - Chapter 6: Flow phenomenon

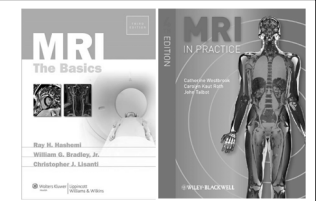


<http://cflu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

2



磁振造影流程

MRI Procedure



Procedure of MRI

- ☒ Alignment (magnetization) B_0
- ☒ Precession $\omega_0 = \gamma B_0$
- ☒ Resonance (given B_1 by RF with ω_2) $\omega_1 = \gamma B_1$, $B_1 \perp B_0$
 - The most effective resonance is produced when $\omega_0 = \omega_2$
- ☒ MR signal (EMF, relaxation time)
- ☒ Imaging (Pulse sequencing: SE, GRE, EPI)
 - ☒ • Tissue Contrast: Image weighting
 - ☒ • Spatial localization: Slice selection & Spatial Encoding
 - ☒ • Data space/K space
- ☐ Tissue Suppression Techniques



<http://cflu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

3


<http://cflu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22


4

組織壓抑技術

Tissue Suppression Techniques



Glioblastoma MRI

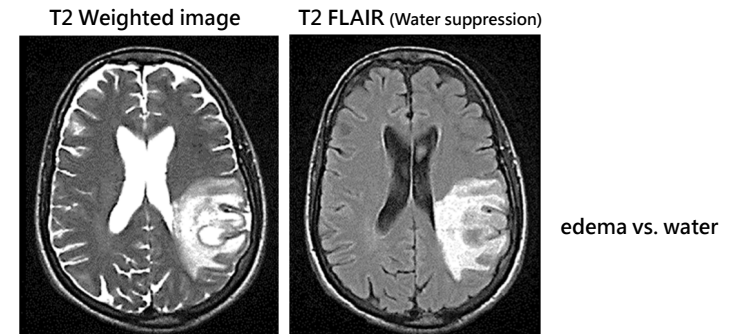


<http://journal.frontiersin.org/article/10.3389/fonc.2013.00066/full>

Breast cancer MRI


T1 Weighted image



T1: $H_2O > \text{Solid tissue} > \text{Fat}$
Gd contrast agent can shorten tissue T1
Fat saturation + Gd enhancement

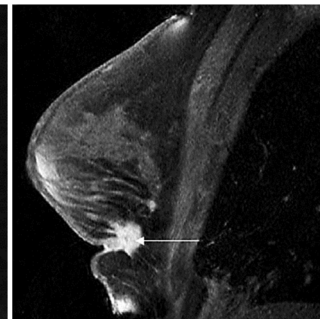

British Journal of Cancer (2003) 88(1), 4-10




Suppression techniques


- To suppress the signal coming from a certain tissue.
 - Two common targets (tissues): fat and water
- Suppression techniques
 - Inversion recovery (IR) techniques
 - Chemical/spectral saturation
 - Dixon method
 - Spatial presaturation
 - Magnetization transfer (MT)

Inversion recovery, IR

- After the 180° RF pulse, the magnetization starts to recover from $-M_0$ instead of zero.
- $T1(\text{null}) = (\ln 2)T1 \approx 0.693 T1$.

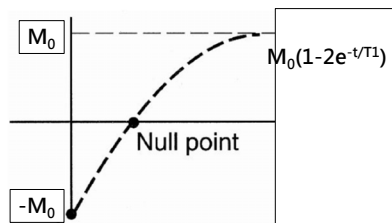

<http://cfliu.lab.nyu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

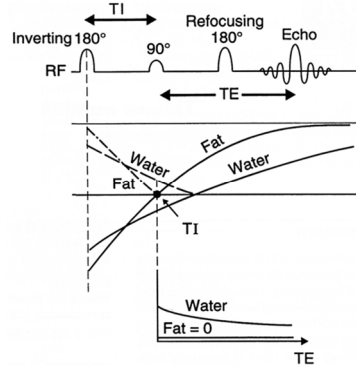


2025/11/22

9

Tissue Suppression: STIR & FLAIR

- STIR: Short tau inversion recovery, fat suppression
 - At 1.5T, $TI = 0.693 \times 200 = 138.6$ msec
- FLAIR: Fluid attenuated inversion recovery, water suppression
 - At 1.5T, $TI = 0.693 \times 3600 = 2494.8$ msec

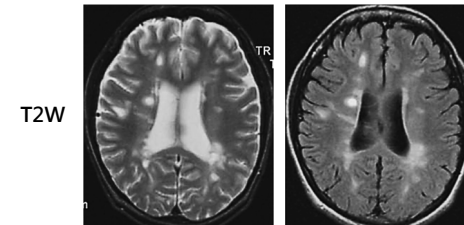


<http://cfliu.lab.nyu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

10

Fast FLAIR: an example

- IR for water + fast spin echo (FSE)
- Multi-slice + FSE
- The maximum # of slice in one TR is usually limited by TI

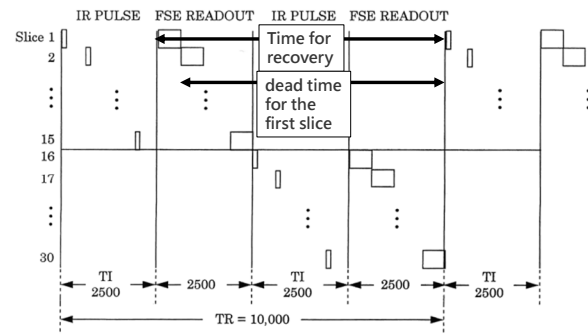

<http://cfliu.lab.nyu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

11

Advantages/Disadvantages of IR


- Advantage
 - No variability caused by magnetic field inhomogeneities
- Disadvantages
 - Tissues with similar T1 values are all suppressed (e.g. Gd effects).
 - Long acquisition times caused by long TRs
 - Cause extra 180° RF heating
 - Low SNR (due to the partial saturation of all tissues)

<http://cfliu.lab.nyu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

12

Water & fat chemical shift

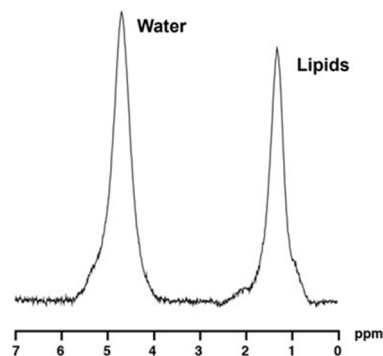


- Peak location
 - Water 4.7 ppm
 - Fat (lipids) 1.3 ppm
 - ppm: parts per million
- $$\omega = 42.6 \times 1.5T = 63.9 \text{ MHz}$$

$$= 42.6 \times 3.0T = 127.8 \text{ MHz}$$
- 1.5T: $(4.7-1.3) \times 63.9 = 217.36 \text{ Hz}$
 - 3.0T: $(4.7-1.3) \times 127.8 = 434.52 \text{ Hz}$

Chemical/spectral presaturation

- A frequency-selective presaturation pulse is applied before the RF excitation pulse.
- CHESS: Chemical shift selective
- We select appropriate frequency (based on the Larmor equation) to suppress fat or water.

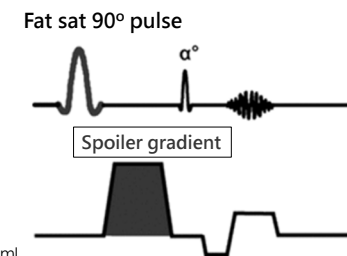

- At 1.5T, water protons precess 210-220 Hz faster than fat protons;
- At 3.0T, water protons precess 420-440 Hz faster than fat protons.


<http://mri-q.com/fat-sat-pulses.html>

Chemical/spectral presaturation

- Advantages
 - Resolves tissues with similar T1 values (fat and Gd-enhanced tumors)
 - No influence on the signal from other tissues (in contrast, IR affects the contrast of all tissues)
- Disadvantages
 - Suffers from sensitivity to magnetic field inhomogeneities (e.g. metallic susceptibility artifacts).
 - Cause extra 90° RF heating
 - May lengthen TR, thus increasing the scan time (5~8 ms)

STIR vs. Fat Sat.

- Endometrioma (aka. chocolate cysts)

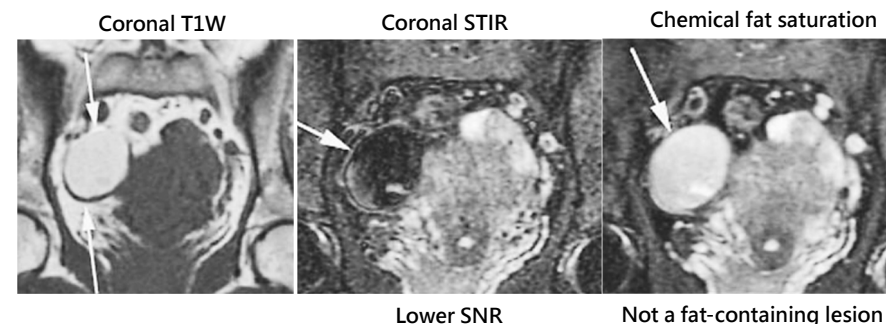

Lower SNR


Not a fat-containing lesion

Dixon Method

- Chemical shift between water and fat
- two sets of SE images were acquired with different echo times
 - the first with fat and water signals in phase (IP) at the center of the echo
 - the second with the TE adjusted by a few milliseconds so that the fat and water signals were out-of-phase (OP).

$$\begin{aligned} \text{IP} &= \text{W} + \text{F} \\ \text{OP} &= \text{W} - \text{F} \end{aligned}$$

$$\begin{aligned} \frac{1}{2}(\text{IP} + \text{OP}) &= \text{W} \\ \frac{1}{2}(\text{IP} - \text{OP}) &= \text{F} \end{aligned}$$

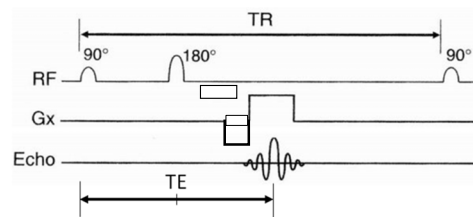


<http://cfliu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

17

Dixon Method

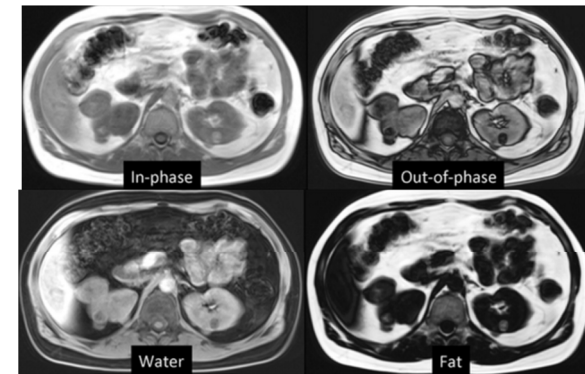


<http://mri-q.com/dixon-method.html>

2025/11/22

18

Fat-water swap

- Generally better than CHES/Fat-Sat sequences
- Modern Dixon methods still have their limitations
 - particularly in highly inhomogeneous areas like the neck and around metal hardware → fat-water swap

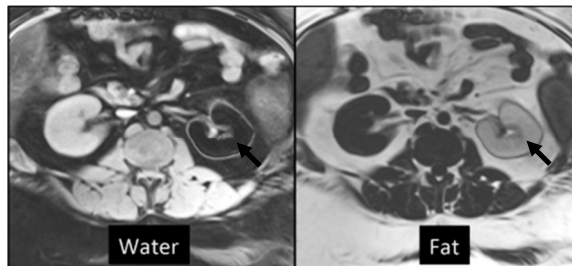


<http://cfliu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

19

Spatial presaturation

- 90° saturation pulses are applied on either side of selected volume (anterior/posterior, superior/inferior, right/left).
- To suppress phase ghosts caused by...
 - Motion artifacts
 - Flow-related artifacts

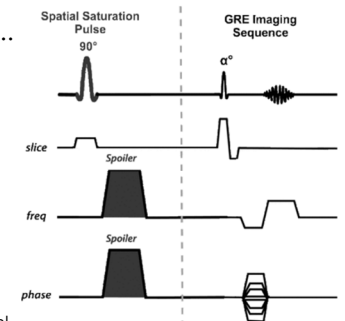

<http://mri-q.com/saturation-pulses.html>


<http://cfliu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

20

Spatial presaturation

- Applications:
 - **Imaging of spine:** a sat. band is placed within the FOV anterior to the vertebral bodies.
 - **MR angiography:** sat. pulses are placed outside the FOV at one end of a vessel to suppress either venous or arterial flow.
 - **MR spectroscopy:** Sat. bands are placed on the skull regions.

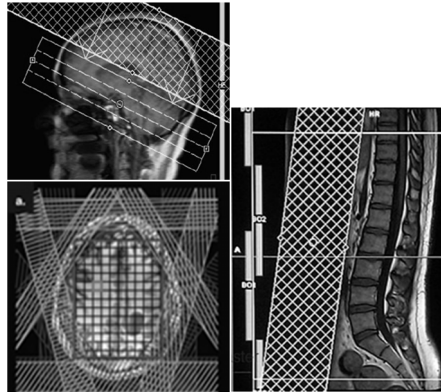


Spatial presaturation

- Advantages
 - Minimize phase ghosts (motion artifacts)
 - Minimize flow artifacts
- Disadvantages
 - May cause signal suppression in the remainder of the FOV
 - May lengthen TR, thus increasing the scan time (5~8 ms)


Non-fatty hydrogen nuclei

- Bulk (free) water
 - T1: 2000~3000 msec
 - T2: 1000~2000 msec
- Hydration layer (bound) water
 - T1: 10~100 msec
 - T2: 5~10 msec
- Macromolecules

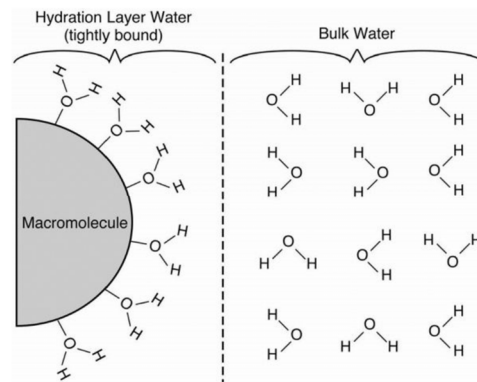

Magnetization transfer, MT

- To suppress protein-bound water
- Protons in protein-bound water exhibit a resonant frequency that is approximately 500 to 2500 Hz away from that of bulk water protons.

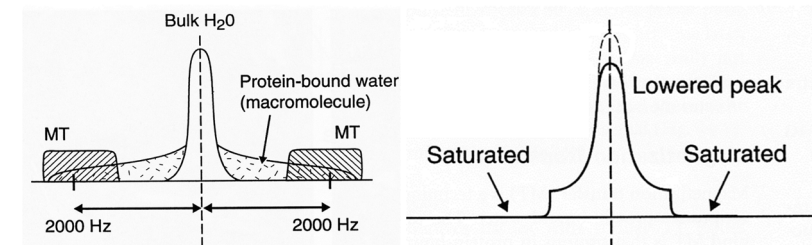

Magnetization transfer, MT

- MT is similar to spectral fat suppression techniques except that here, the off-resonant frequency is up to 2000 Hz as opposed to 220 Hz in the case of fat suppression.
- Used in time of flight (TOF) MR angiography to suppress the background brain tissue and enhance visualization of smaller vessels





<http://cfliu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

25

Procedure of MRI

- ☒ Alignment (magnetization) B_0
- ☒ Precession $\omega_0 = \gamma B_0$
- ☒ Resonance (given B_1 by RF with ω_2) $\omega_1 = \gamma B_1$, $B_1 \perp B_0$
 - The most effective resonance is produced when $\omega_0 = \omega_2$
- ☒ MR signal (EMF, relaxation time)
- ☒ Imaging (Pulse sequencing: SE, GRE, EPI)
 - ☒ • Tissue Contrast: Image weighting
 - ☒ • Spatial localization: Slice selection & Spatial Encoding
 - ☒ • Data space/K space
- ☒ Tissue Suppression Techniques



<http://cfliu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

26

THE END

alvin4016@nycu.edu.tw

<http://cfliu.lab.nycu.edu.tw>, Textbook: MRI The Basics, Hashemi et al.

2025/11/22

27